

1/13

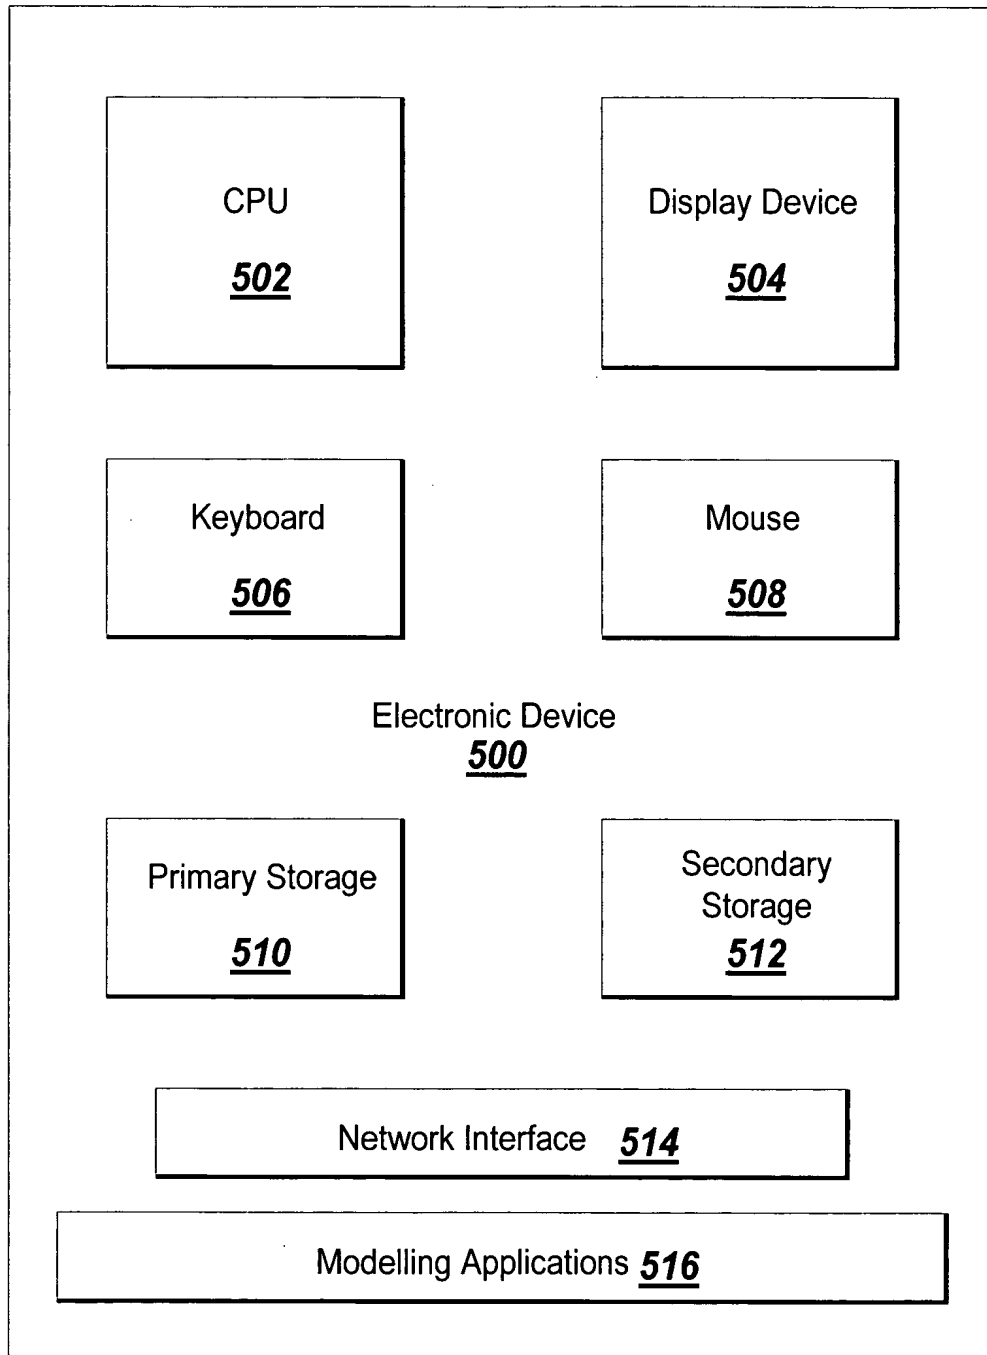


Fig. 1

2/13

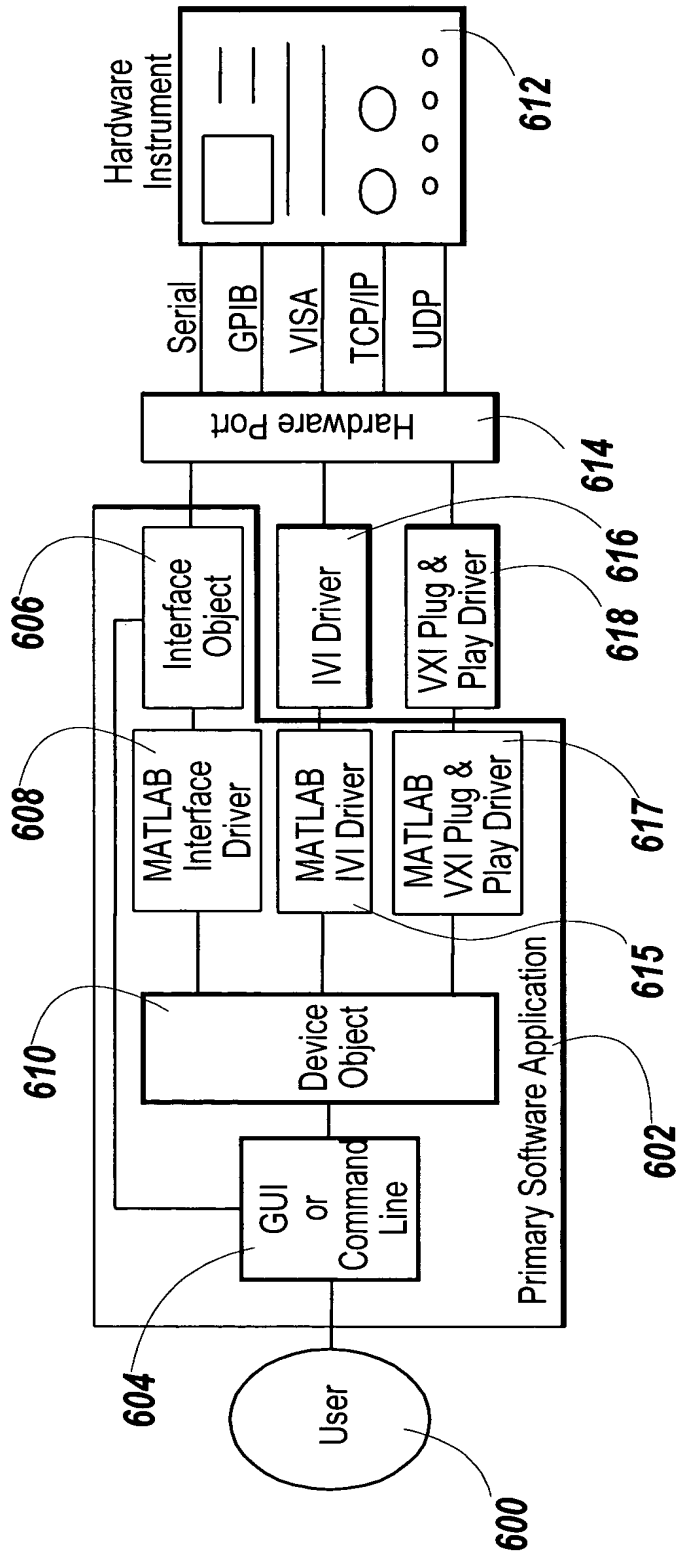


Fig. 2

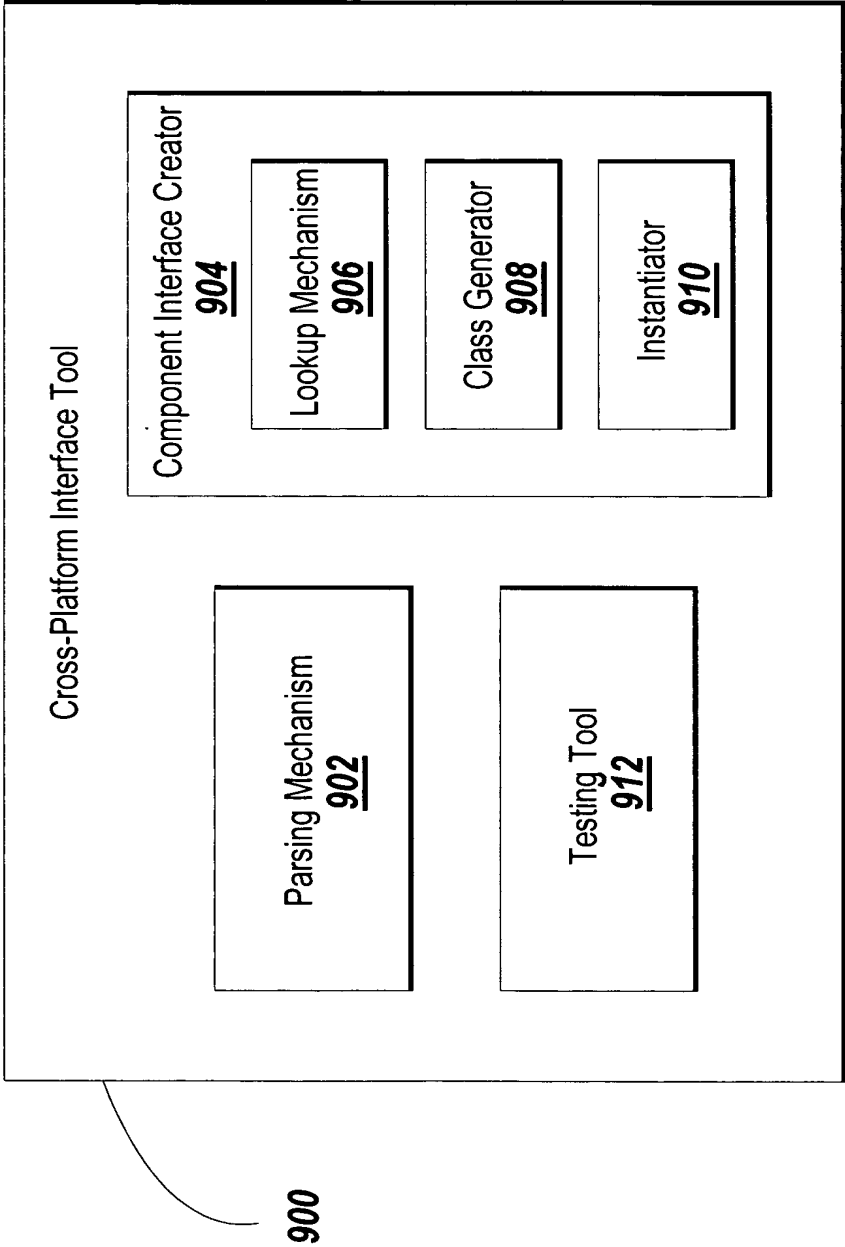


Fig. 3

4/13

630

Block Parameters: Device Object Execute Function

Description

Execute a device object function.

632

Parameters

Block sample time: 1

634

Device Object Instrument Initialization

Name: Unnamed test

636

Driver: D:\tek.mdd Browse...

638

Function:

Device object functions:

- calibrate
- configureWaveform
- devicereset

Function definition: [OUT1] = INVOKE(OBJ, 'calibrate')

Object: Device object

640

OK Cancel Help Apply

Fig. 4

5/13

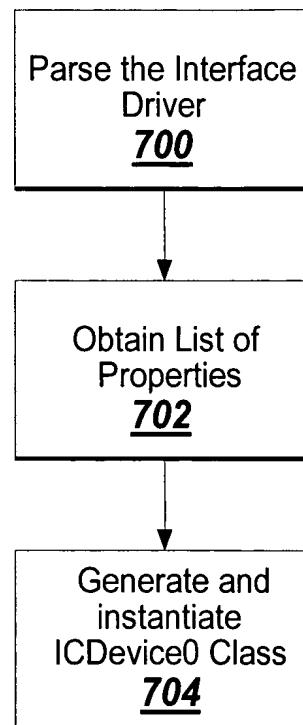


Fig. 5

6/13

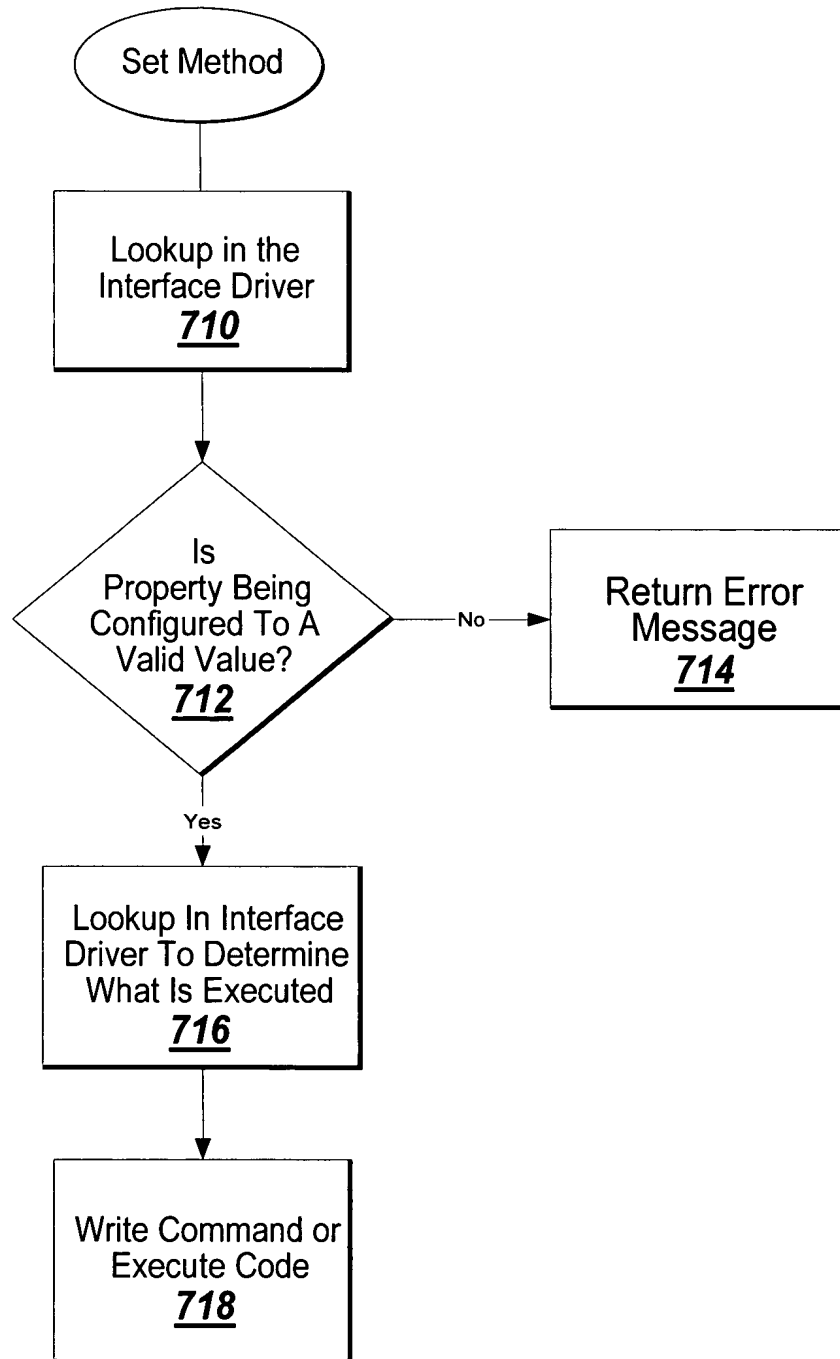


Fig. 6

7/13

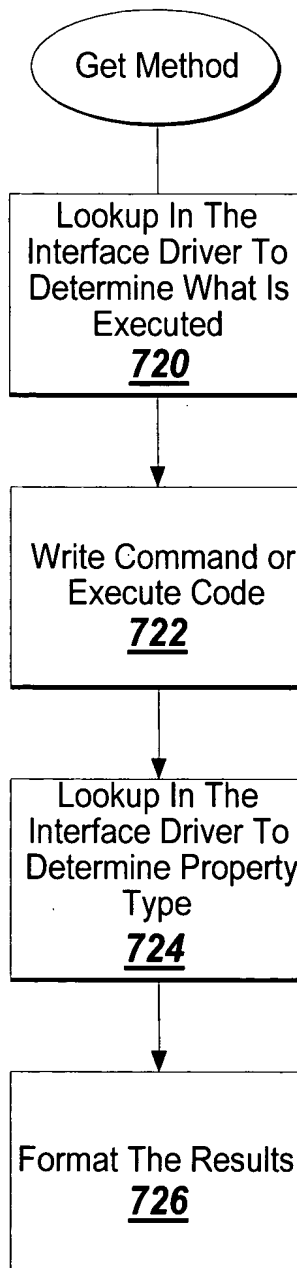


Fig. 7

8/13

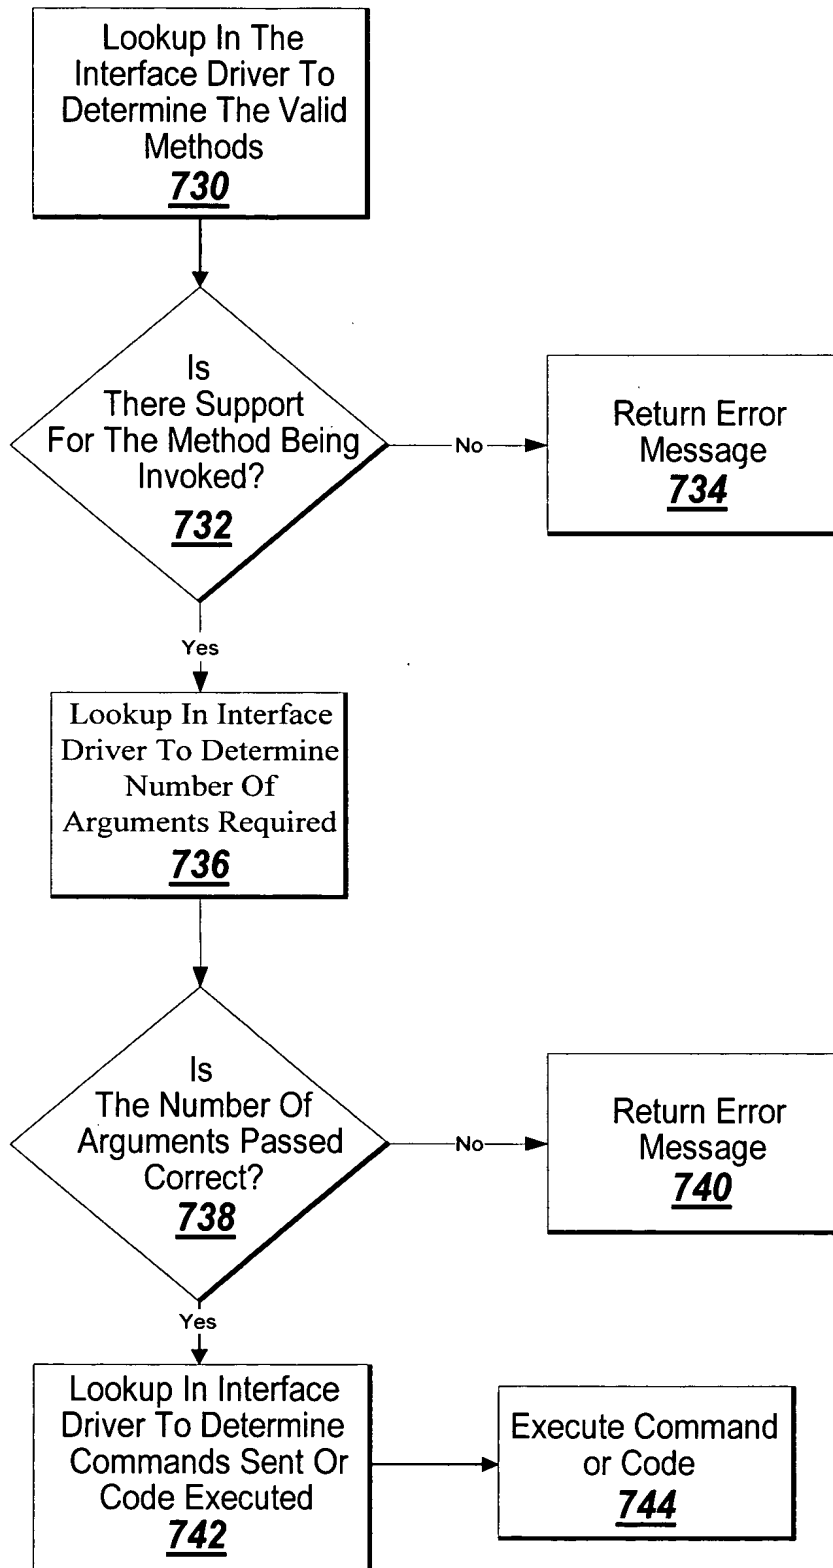


Fig. 8

9/13

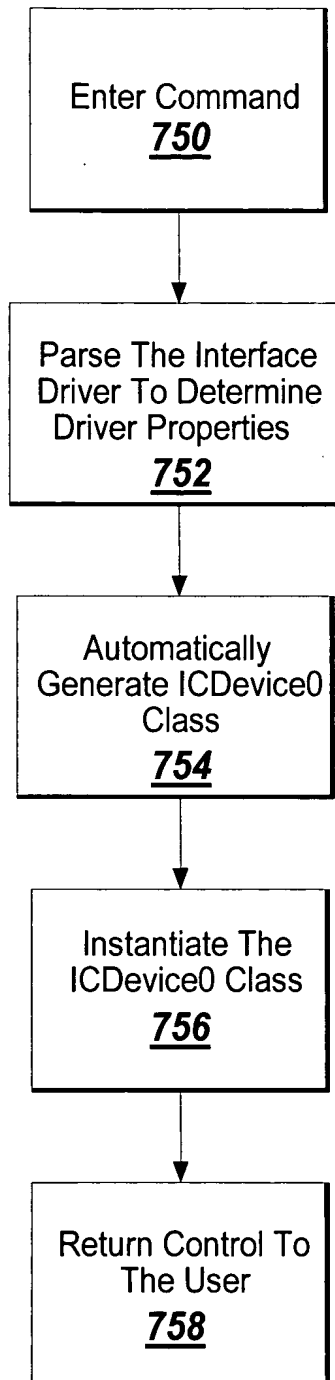


Fig. 9

10/13

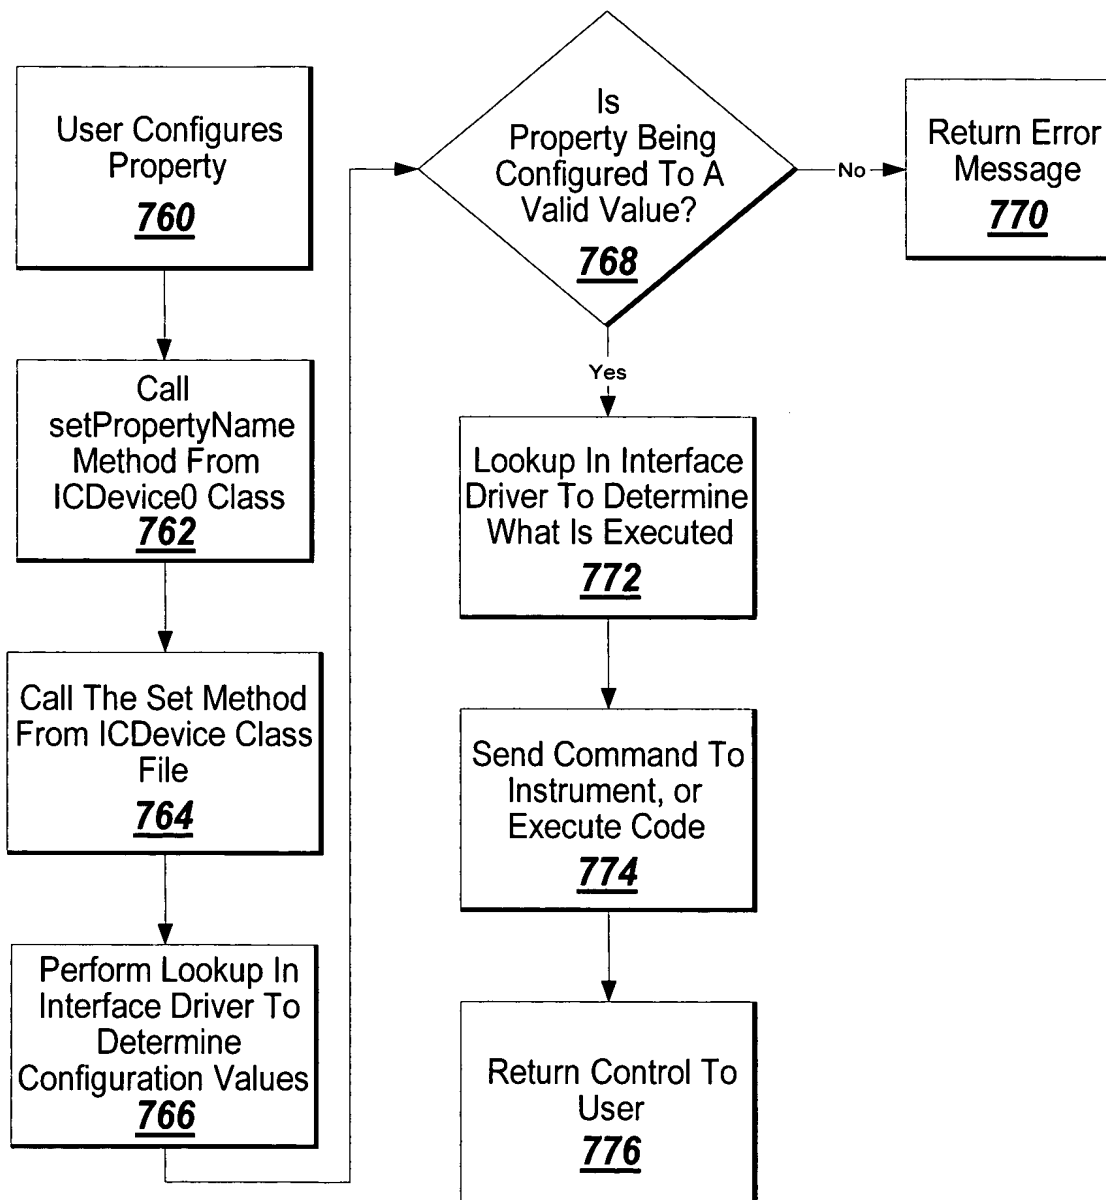


Fig. 10

11/13

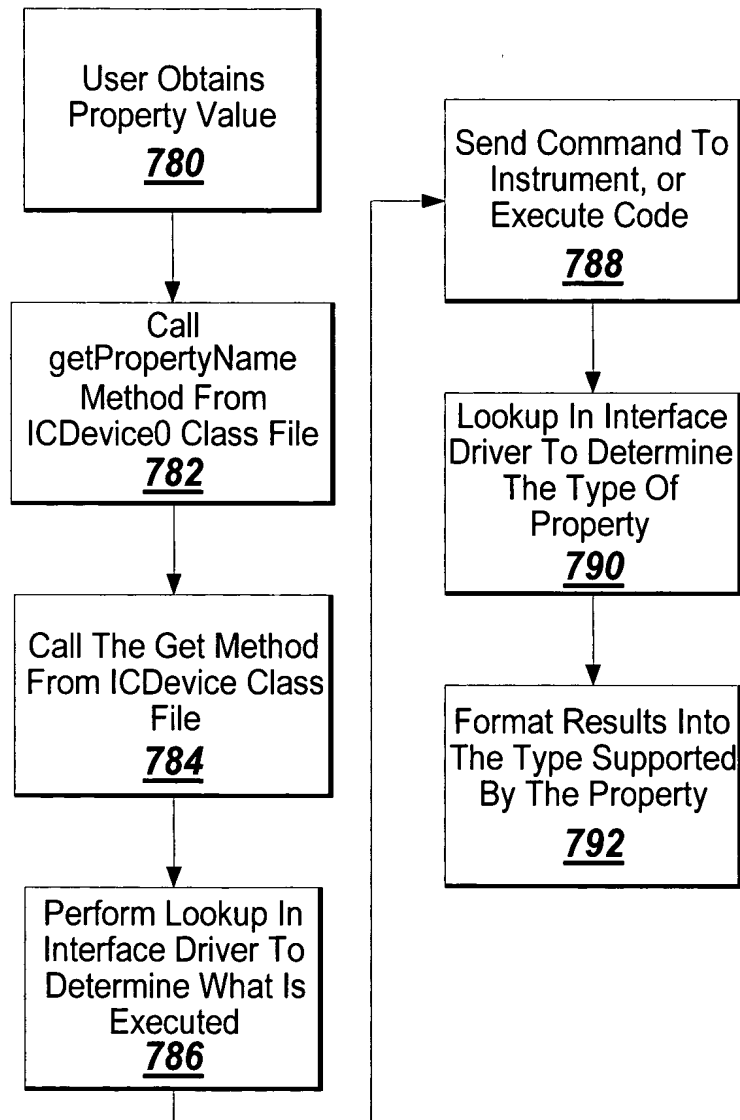


Fig. 11

12/13

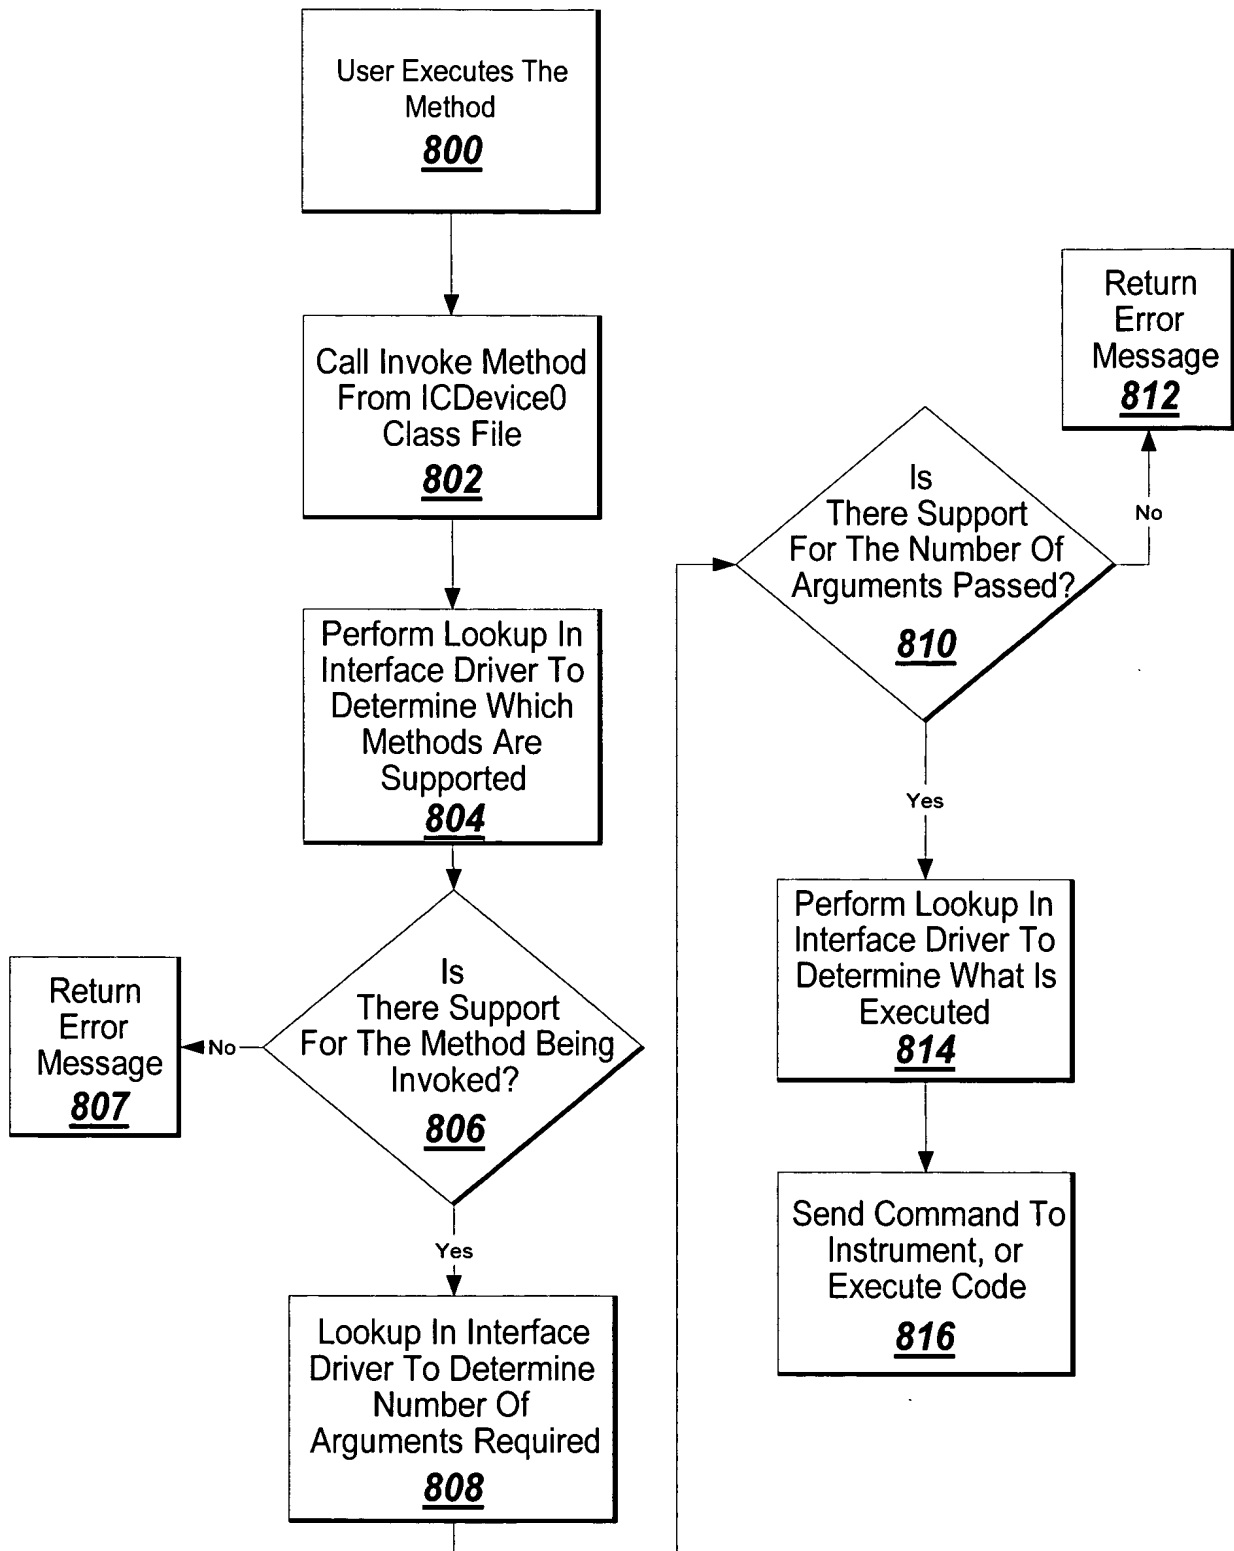


Fig. 12

13/13

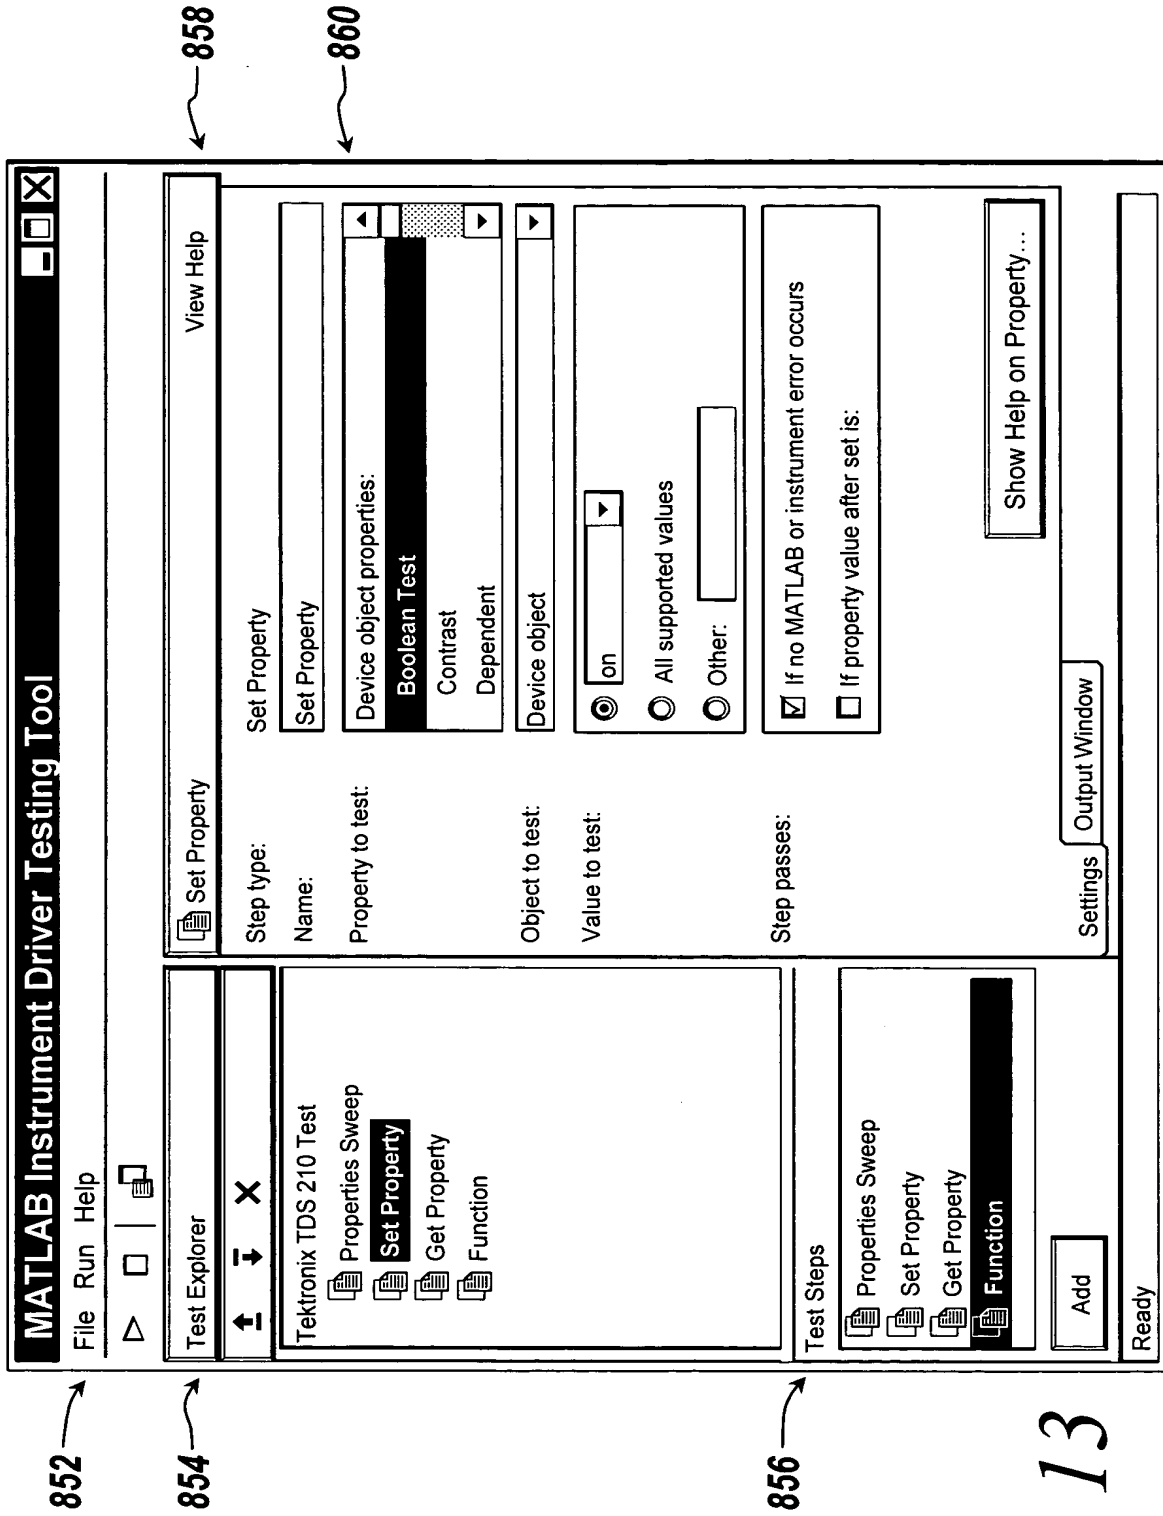


Fig. 13